

CBC-3D[®]

for Abacus

HEMATOLOGY CONTROLS

CONTROL

ASSAY VALUES AND EXPECTED RANGES

QCP DATA MONTHS: **FEBRUARY, MARCH, APRIL****LOT** B0223


2023-05-05

Instrument	Parameter	Low		Normal		High	
		LOT	B0223L	LOT	B0223N	LOT	B0223H
Abacus 3CP	WBC × 10 ⁹ /L		2.0 ± 0.5		7.8 ± 1.2		20.9 ± 2.4
	LYM × 10 ⁹ /L		1.2 ± 0.3		2.6 ± 0.6		3.3 ± 1.5
	MID × 10 ⁹ /L		0.2 ± 0.2		0.7 ± 0.5		1.5 ± 1.4
	GRA × 10 ⁹ /L		0.6 ± 0.2		4.5 ± 0.7		16.1 ± 1.7
	LYM %		62.0 ± 11.0		33.5 ± 7.0		16.0 ± 7.0
	MID %		9.5 ± 9.5		8.5 ± 6.0		7.0 ± 6.5
	GRA %		28.5 ± 9.0		58.0 ± 8.0		77.0 ± 8.0
	RBC × 10 ¹² /L		2.25 ± 0.25		4.52 ± 0.30		5.86 ± 0.35
	HGB g/dL		6.1 ± 0.6		13.7 ± 0.8		18.9 ± 1.2
	HCT %		18.0 ± 2.0		41.1 ± 2.4		57.4 ± 3.0
	MCV fL		80.0 ± 5.0		91.0 ± 5.0		98.0 ± 5.0
	MCH pg		27.1 ± 2.4		30.3 ± 2.8		32.3 ± 2.8
	MCHC g/dL		33.9 ± 3.0		33.3 ± 3.0		32.9 ± 3.0
	RDW CV %		18.5 ± 5.0		17.0 ± 5.0		16.5 ± 5.0
	PLT × 10 ⁹ /L		65 ± 30		248 ± 50		510 ± 60
	MPV fL		9.6 ± 3.0		10.0 ± 3.0		10.5 ± 3.0

Before using, refer to the instruction sheet for mixing directions.

For technical assistance in the USA and Canada call Technical Service at (800) 523-3395.

All brands and products are trademarks or registered trademarks of their respective companies.

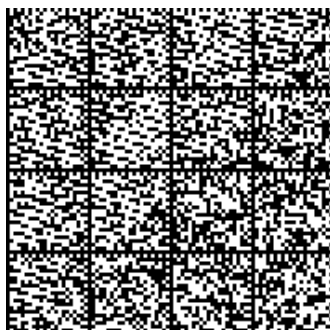

R&D Systems, Inc.
 614 McKinley Place NE
 Minneapolis, MN USA 55413
 AS153-002 Rev. 04/14